


# Water Quality Monitor


## Q46-85 Peracetic Acid Monitor

### STANDARD SYSTEM

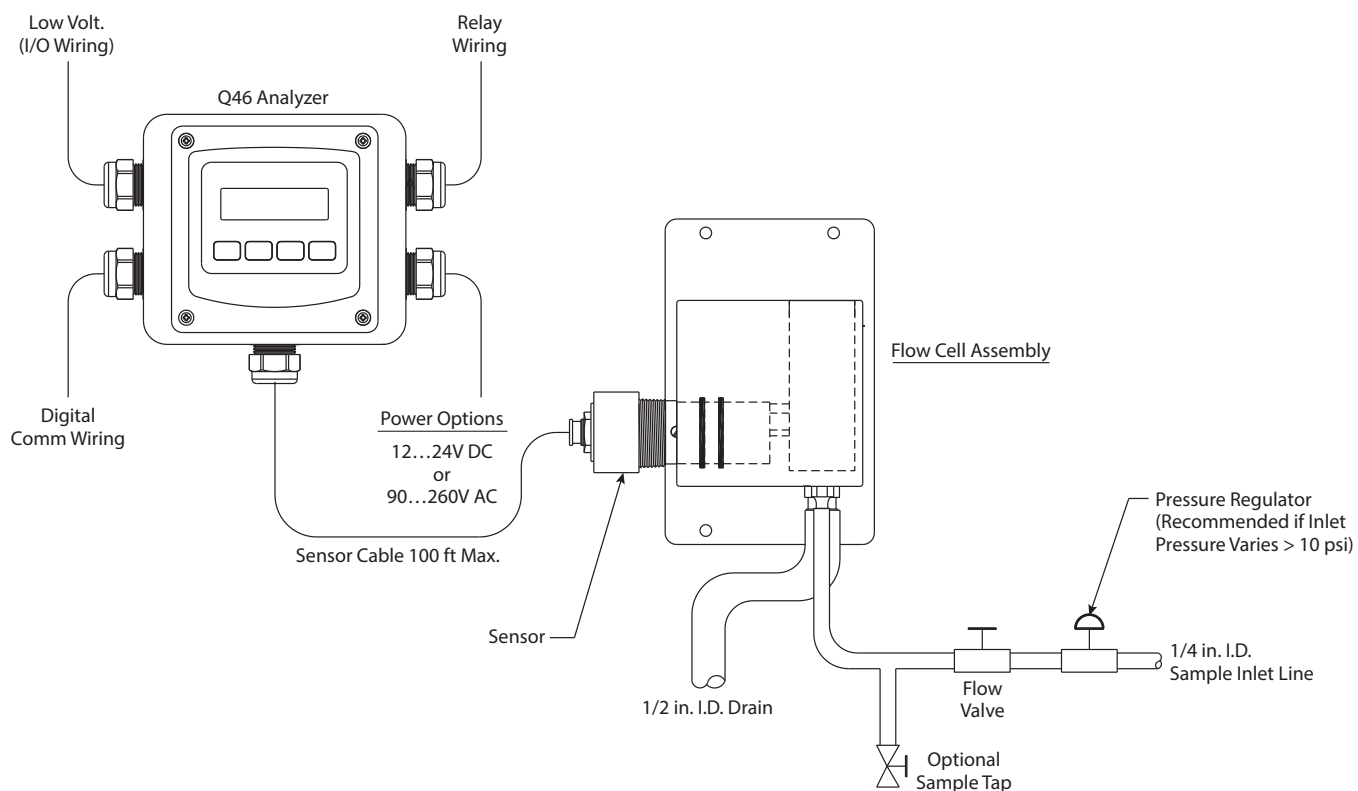


ATI-0922

## SYSTEM DIAGRAM WITH OPTIONAL PH SENSOR

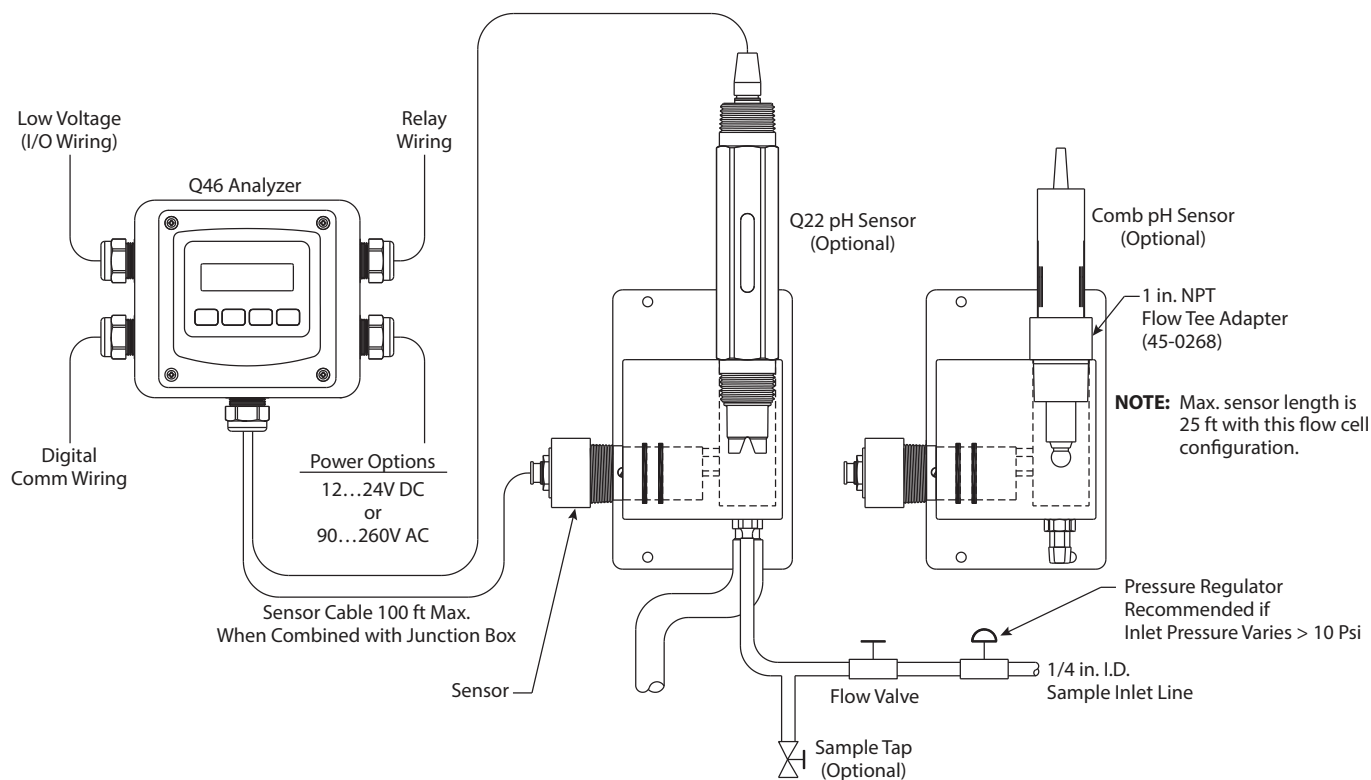


ATi-0923

STANDARD DIAGRAM WITH SEALED FLOWCELL

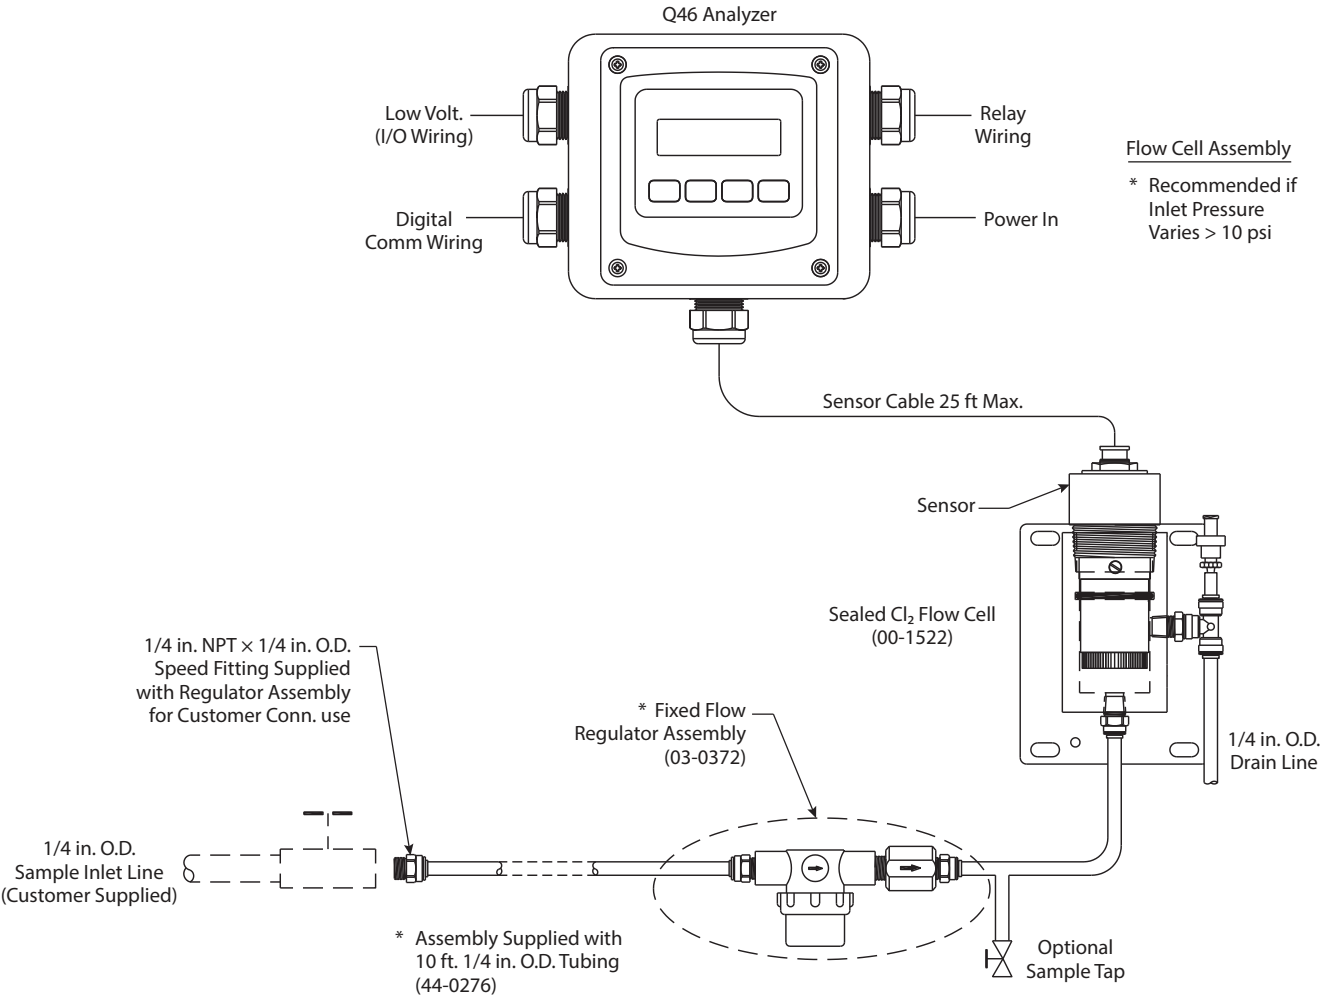


ATi-0924

SYSTEM MOUNTING PLATE ASSEMBLY

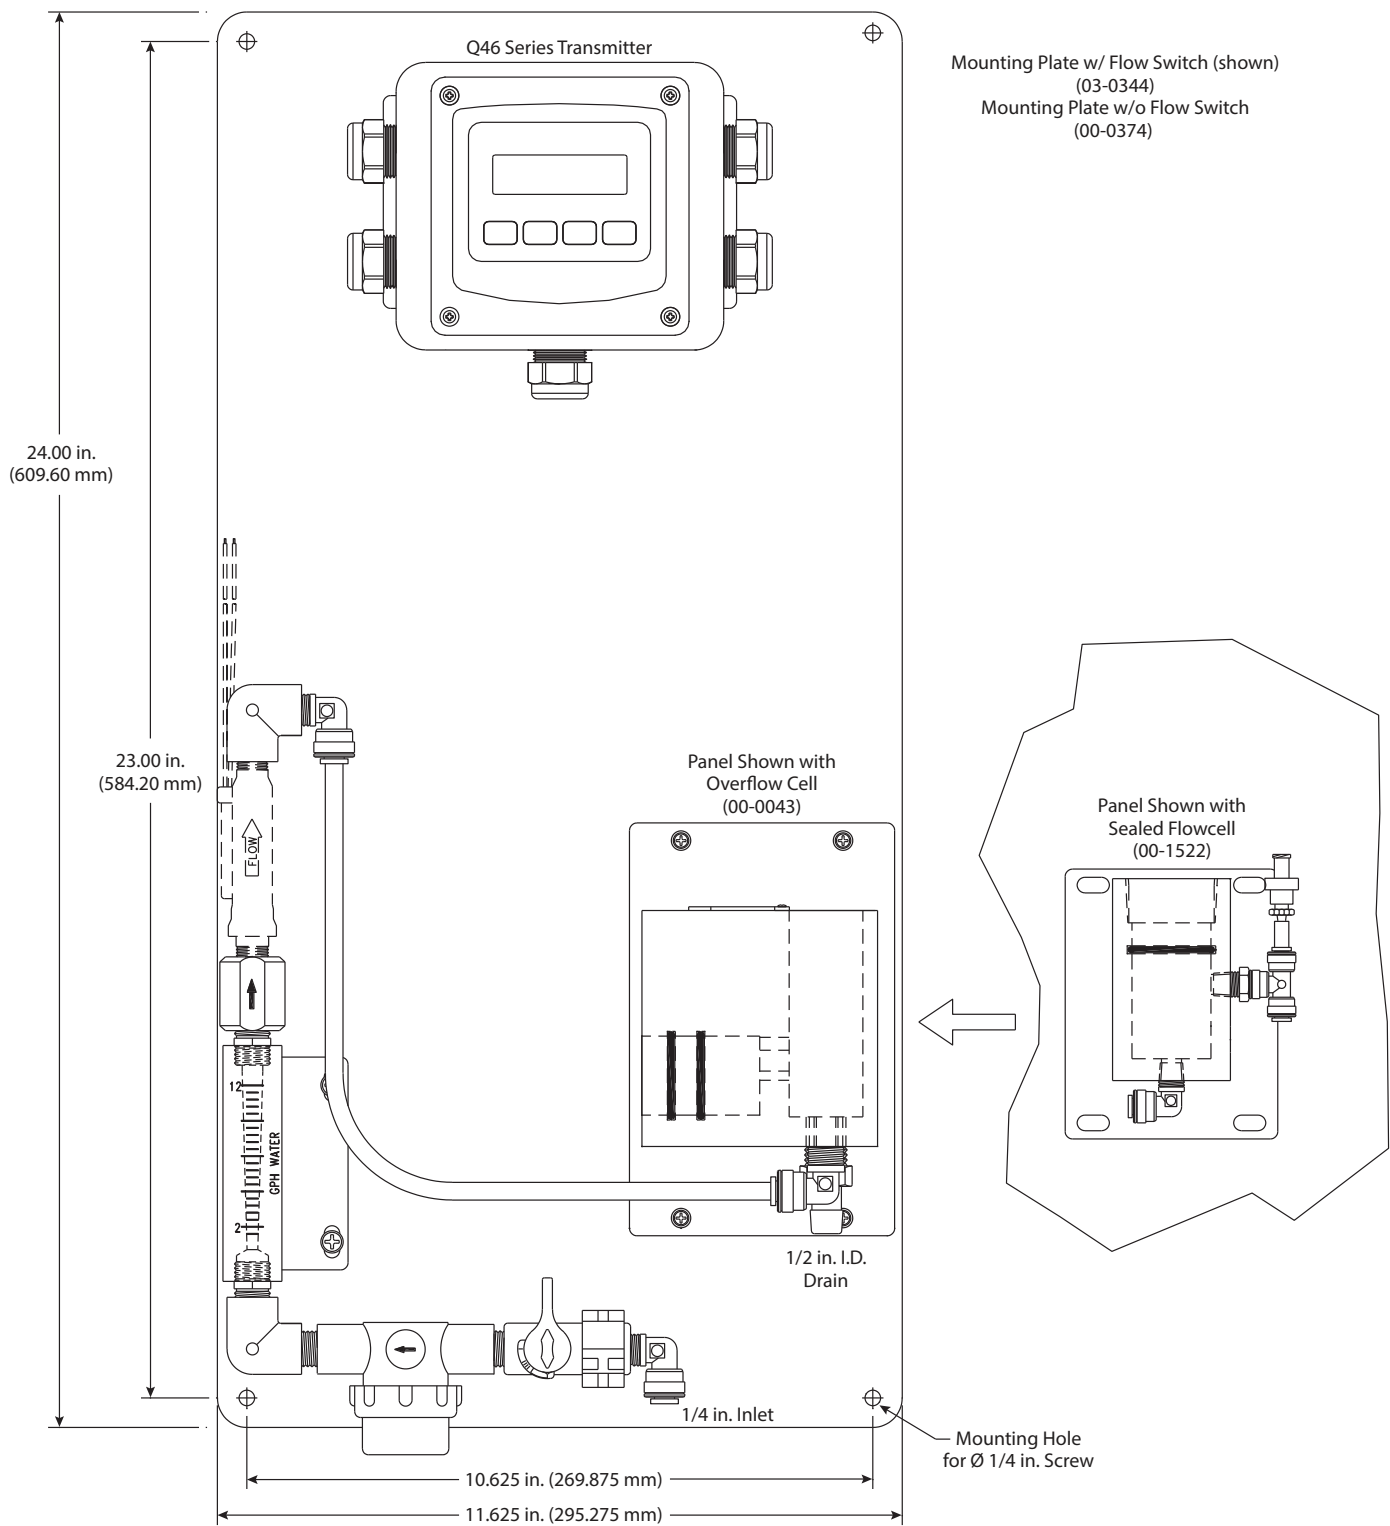


ATI-1224

**ANALYZER DIMENSIONS (WALL MOUNT SHOWN)**

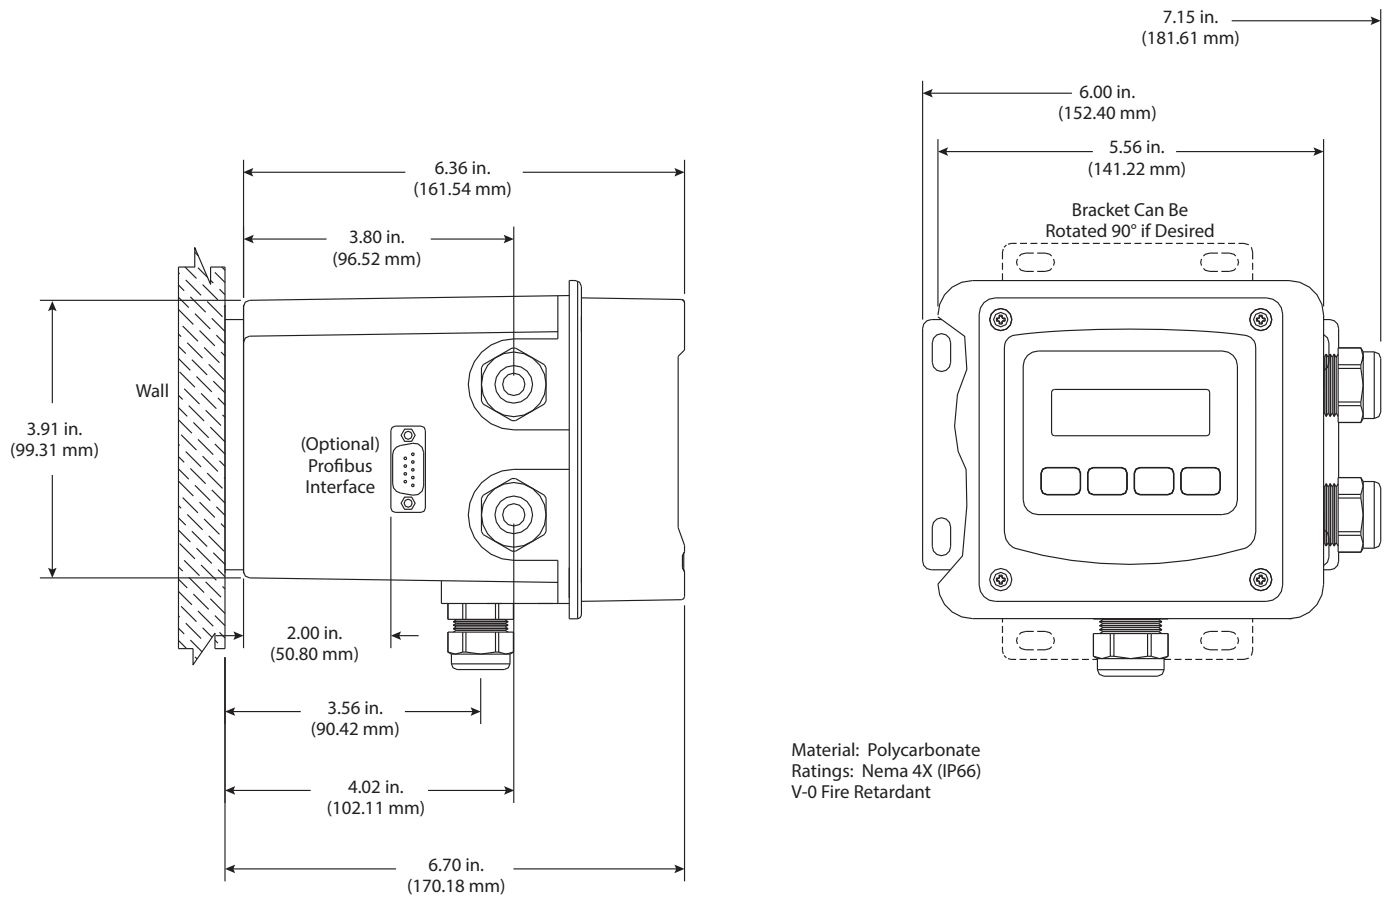


ATi-0926

**JUNCTION BOX**

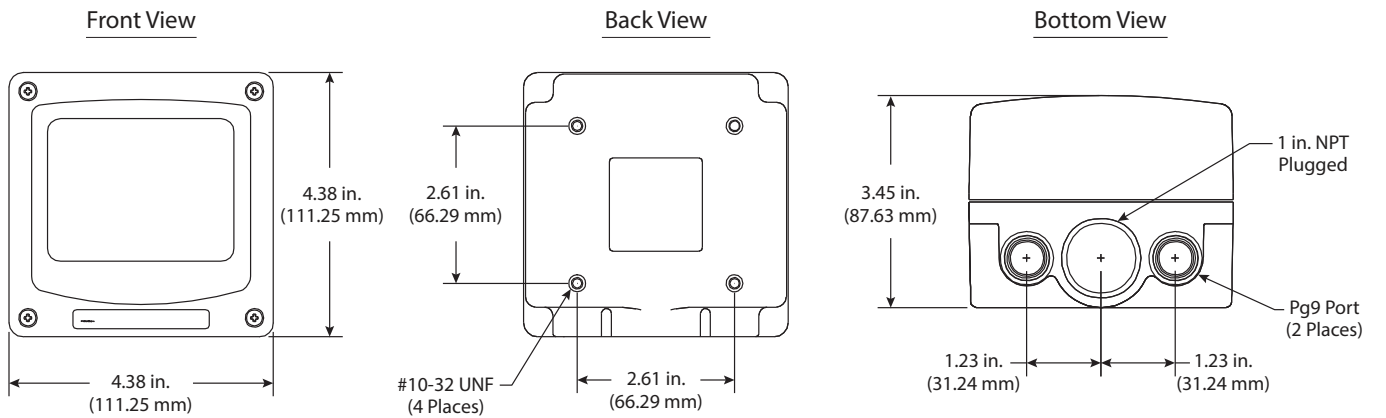


ATi-0655

PIPE MOUNTING

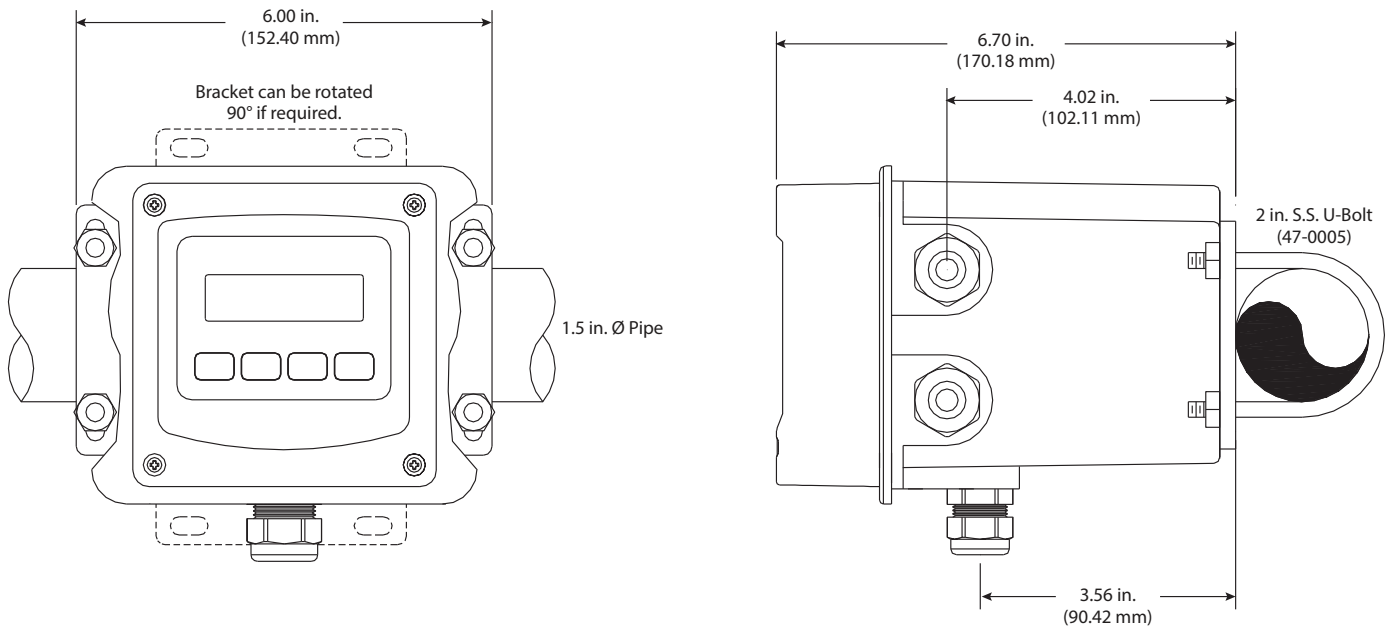


ATi-0927

PANEL MOUNTING

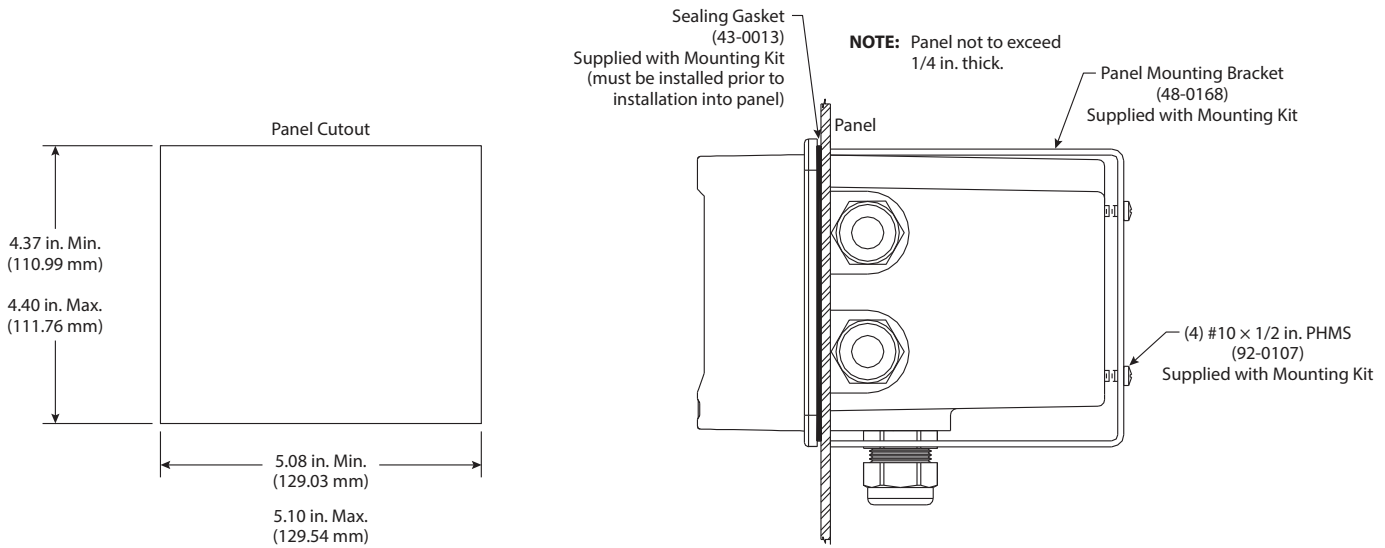


ATi-0928

FLOW SENSOR DIMENSIONS AND OVERFLOW CELL INSTALLATION

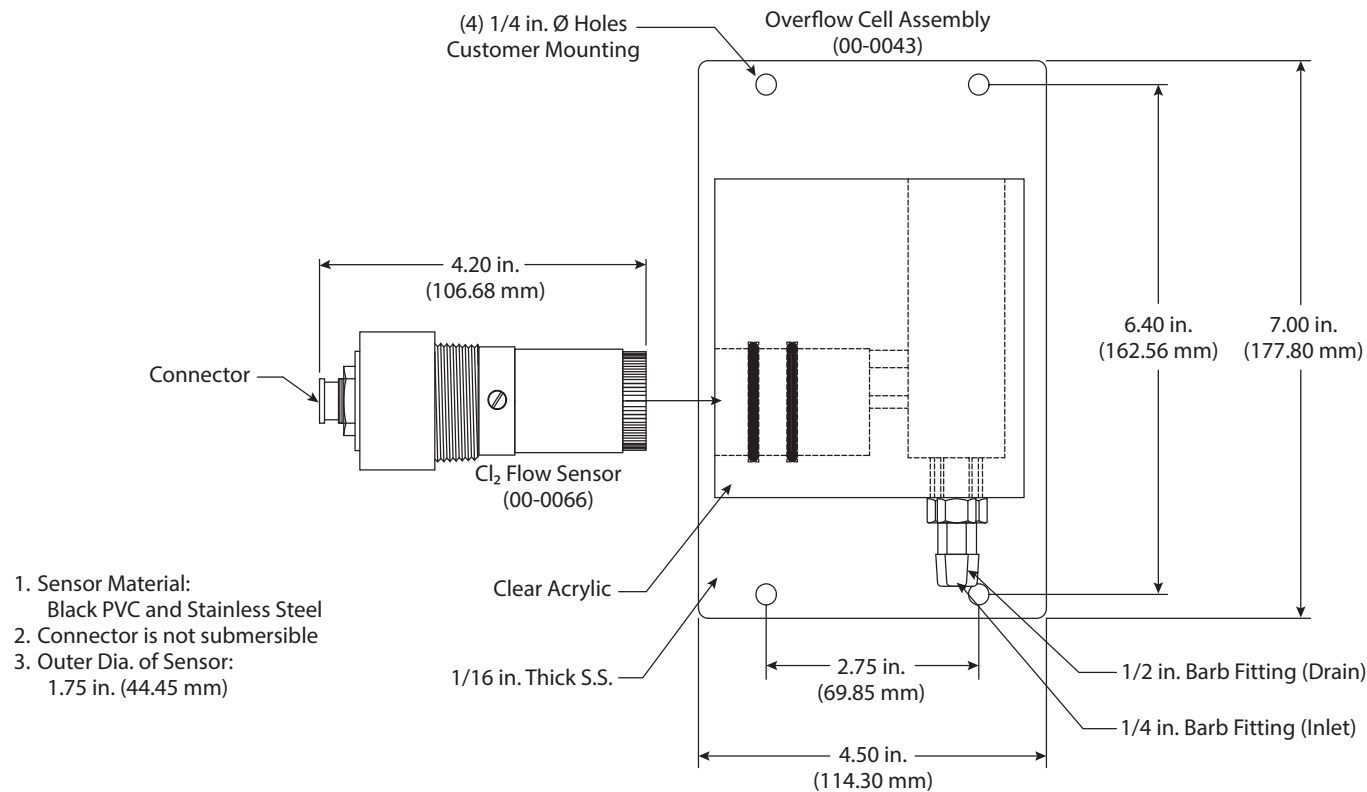


ATi-0196

## CL2 SEALED FLOW CELL (00-1522) DIMENSIONS

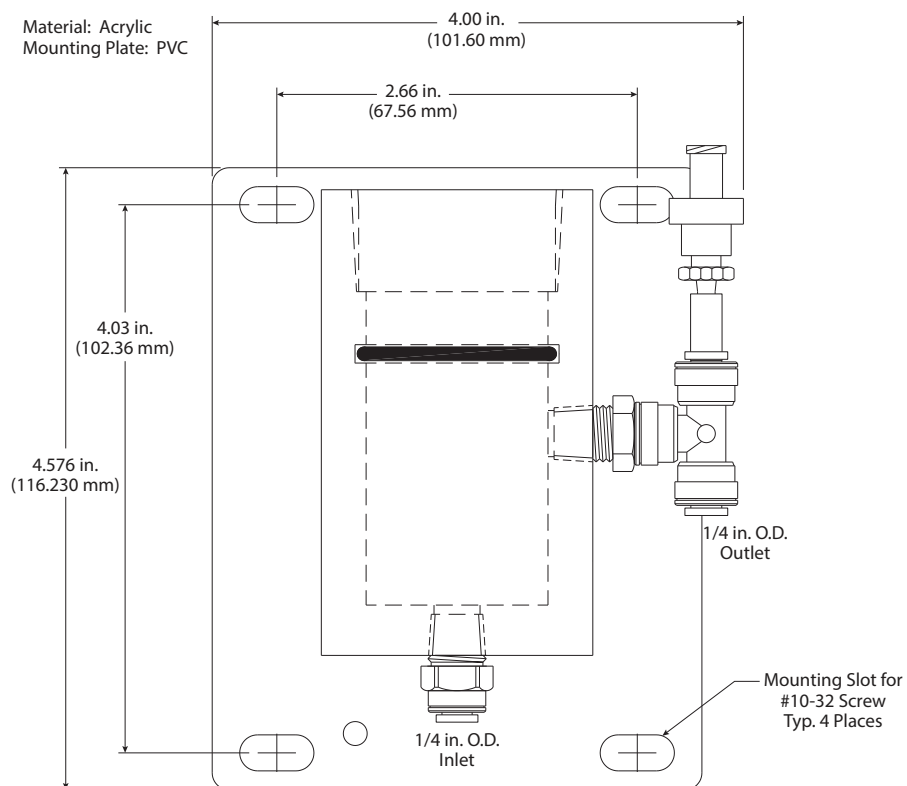


## PH SEALED FLOW CELL ASSEMBLY (00-1527) DIMENSIONS

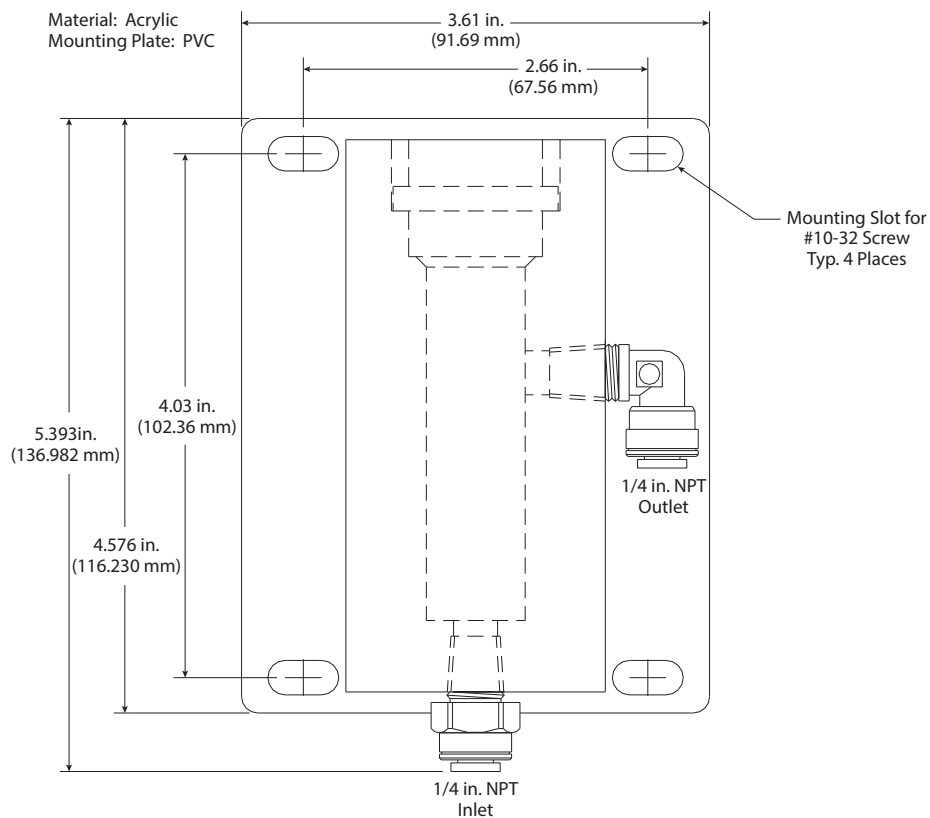




SUBMERSIBLE SENSOR DIMENSIONS

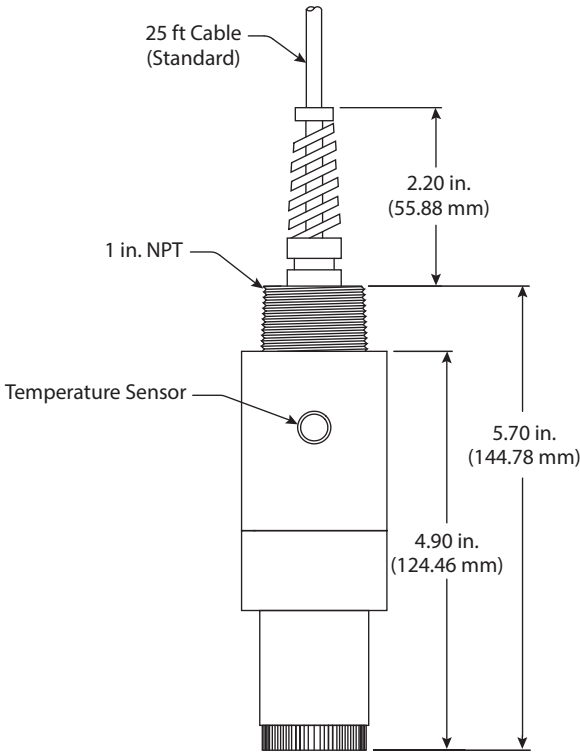


ATi-004

SUBMERSIBLE SENSOR INSTALLATION

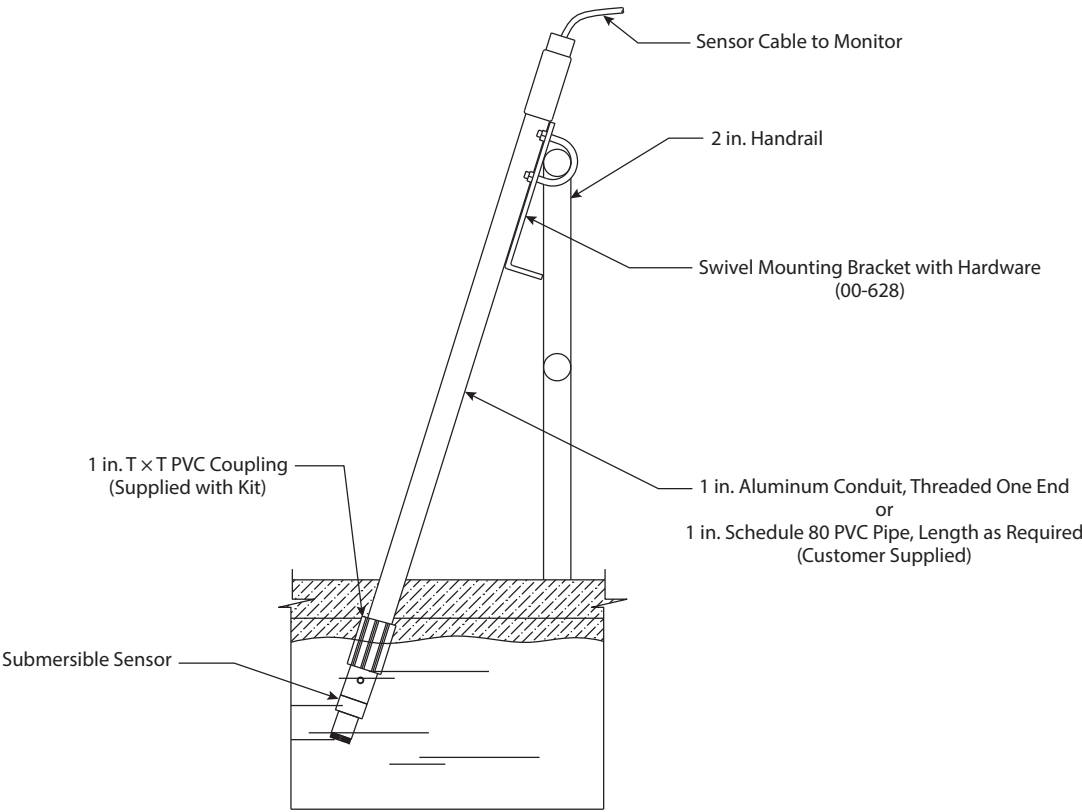


ATi-0155

POWER, RELAY AND OUTPUT CONNECTIONS

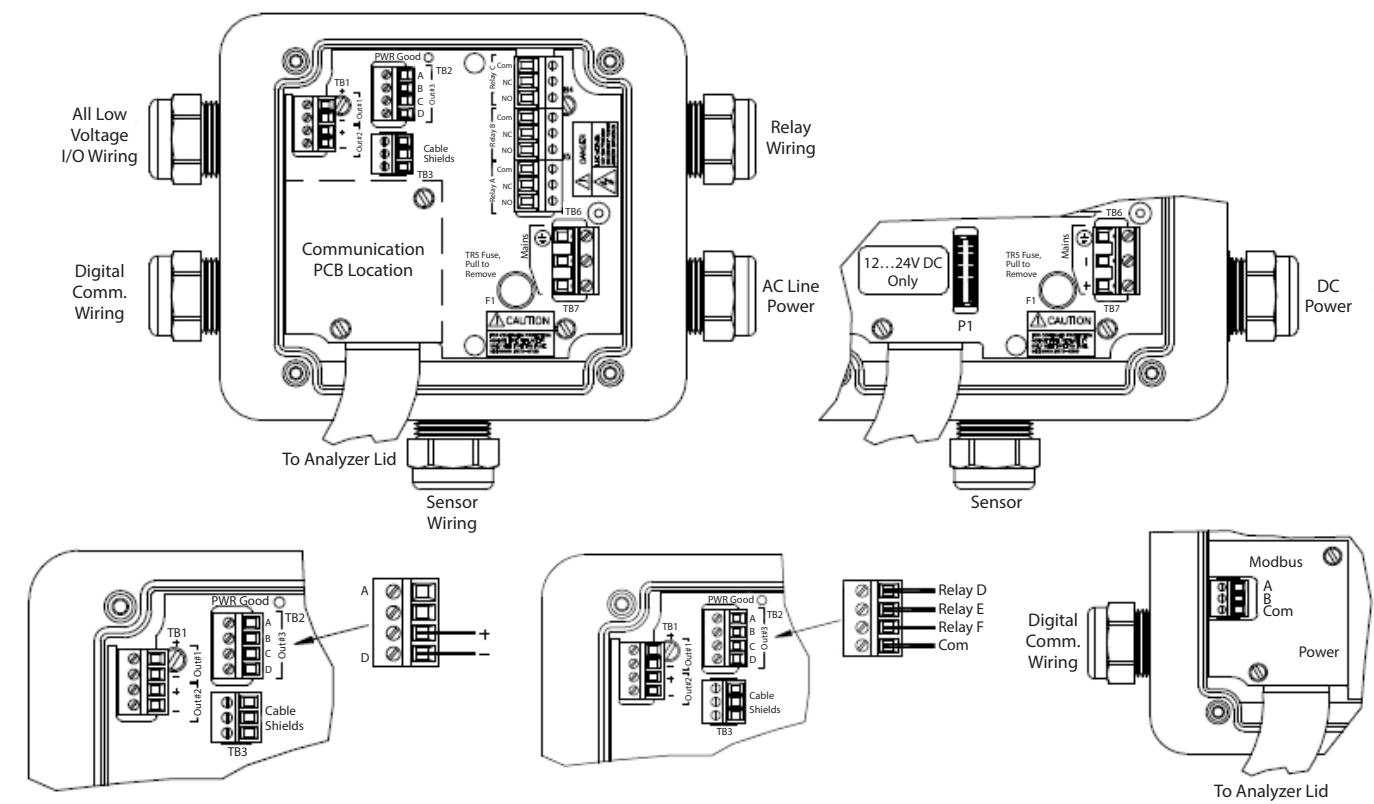


ATi-0930, -0932, -0933, -0989

RELAY WIRING TB4, 5, 6 DETAIL

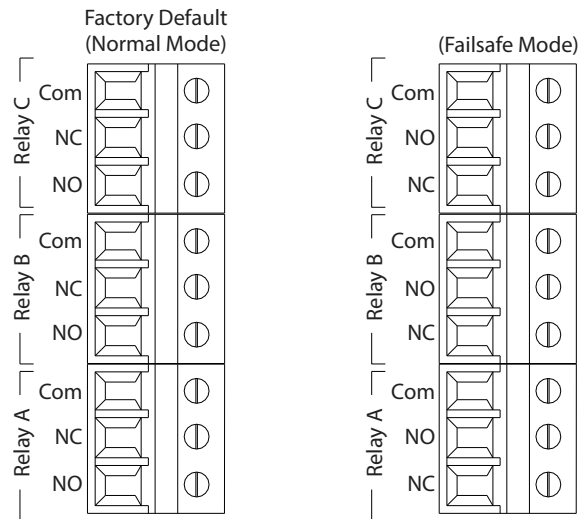


ATi-0931

ELECTRICAL CONNECTIONS

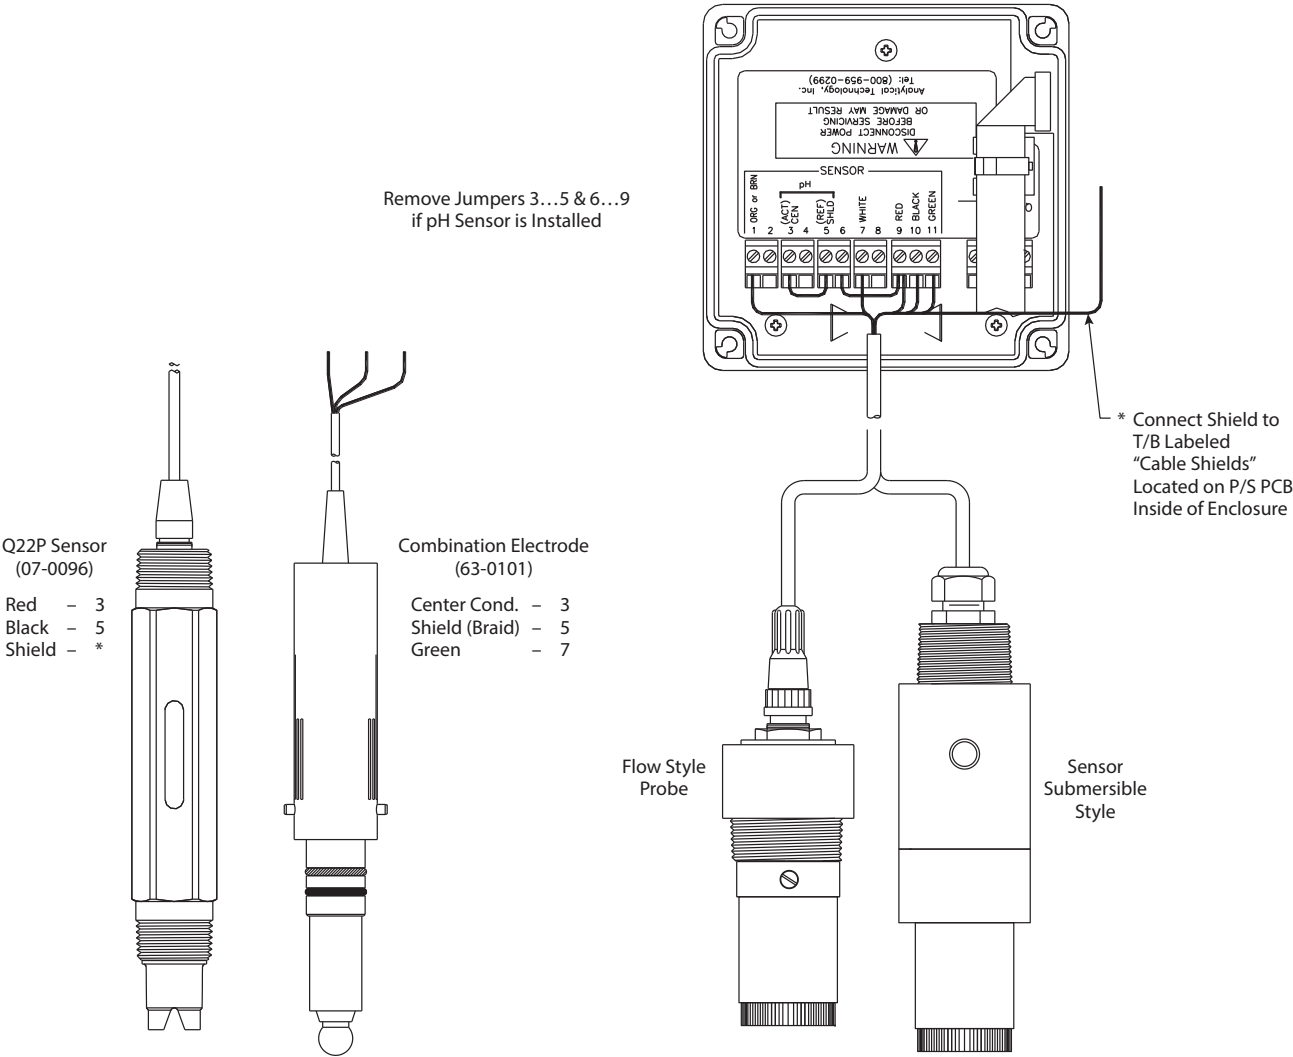

ATi-0929


REMOTE JUNCTION BOX SENSOR CONNECTIONS

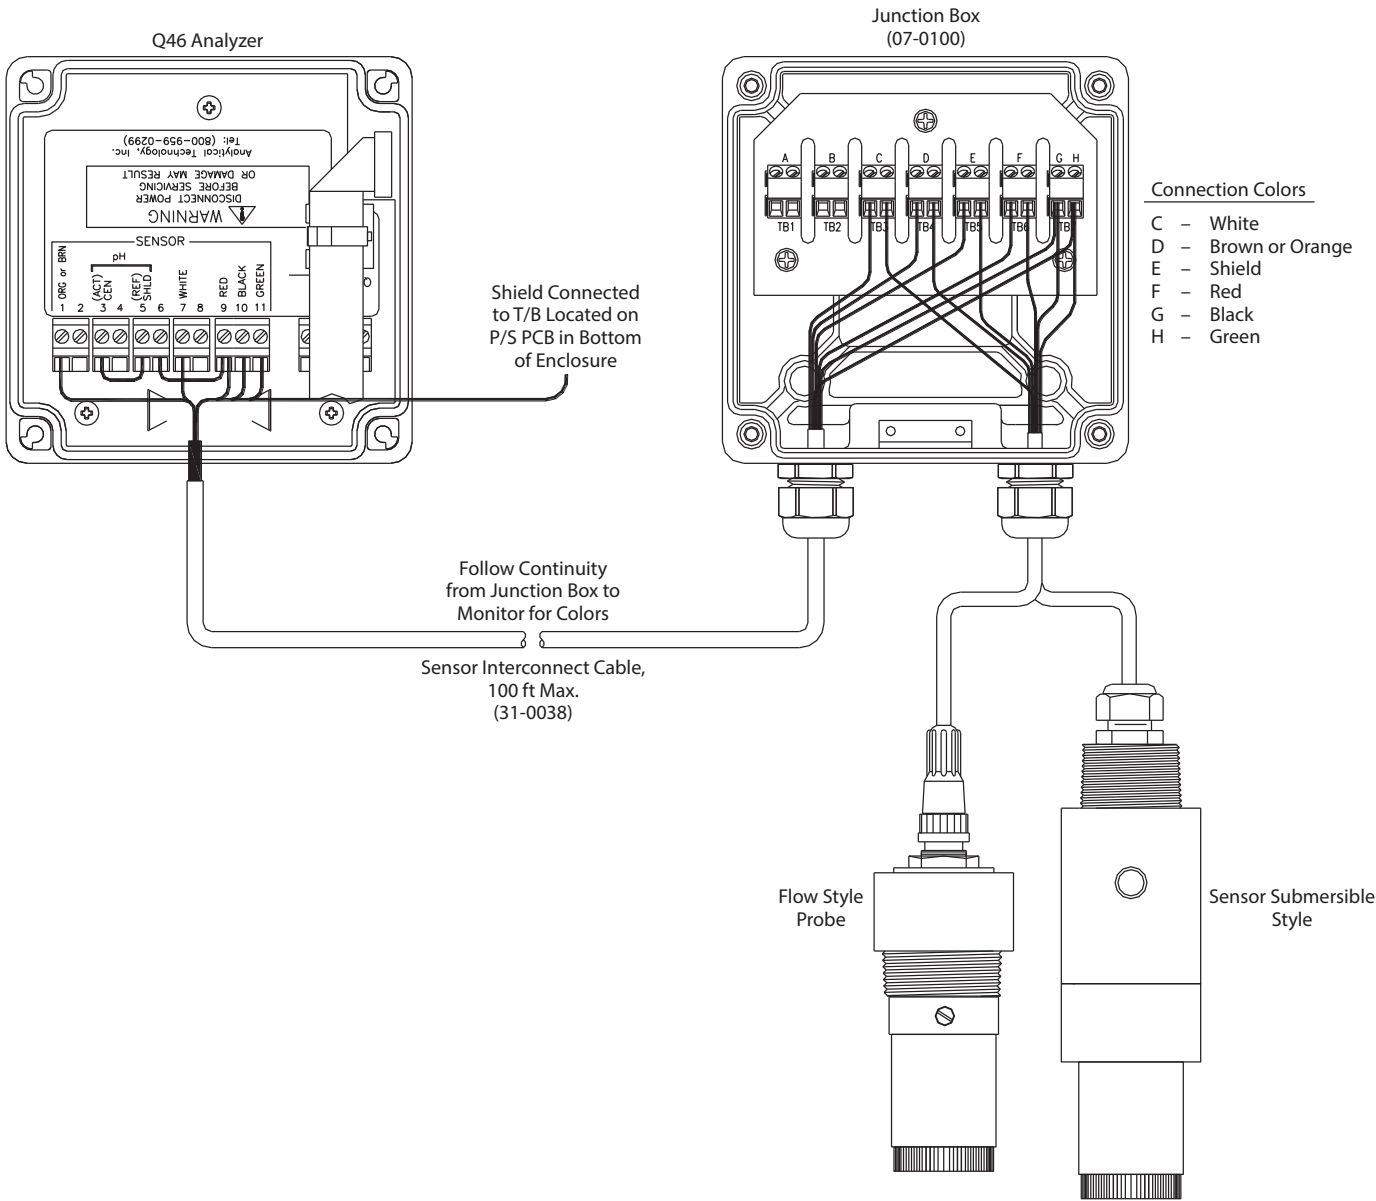

ATi-0934

CL2 PH WITH JUNCTION BOX SENSOR CONNECTIONS

**NOTE:** Bayonet Style Probe (63-0101) CANNOT be used in a remote application.

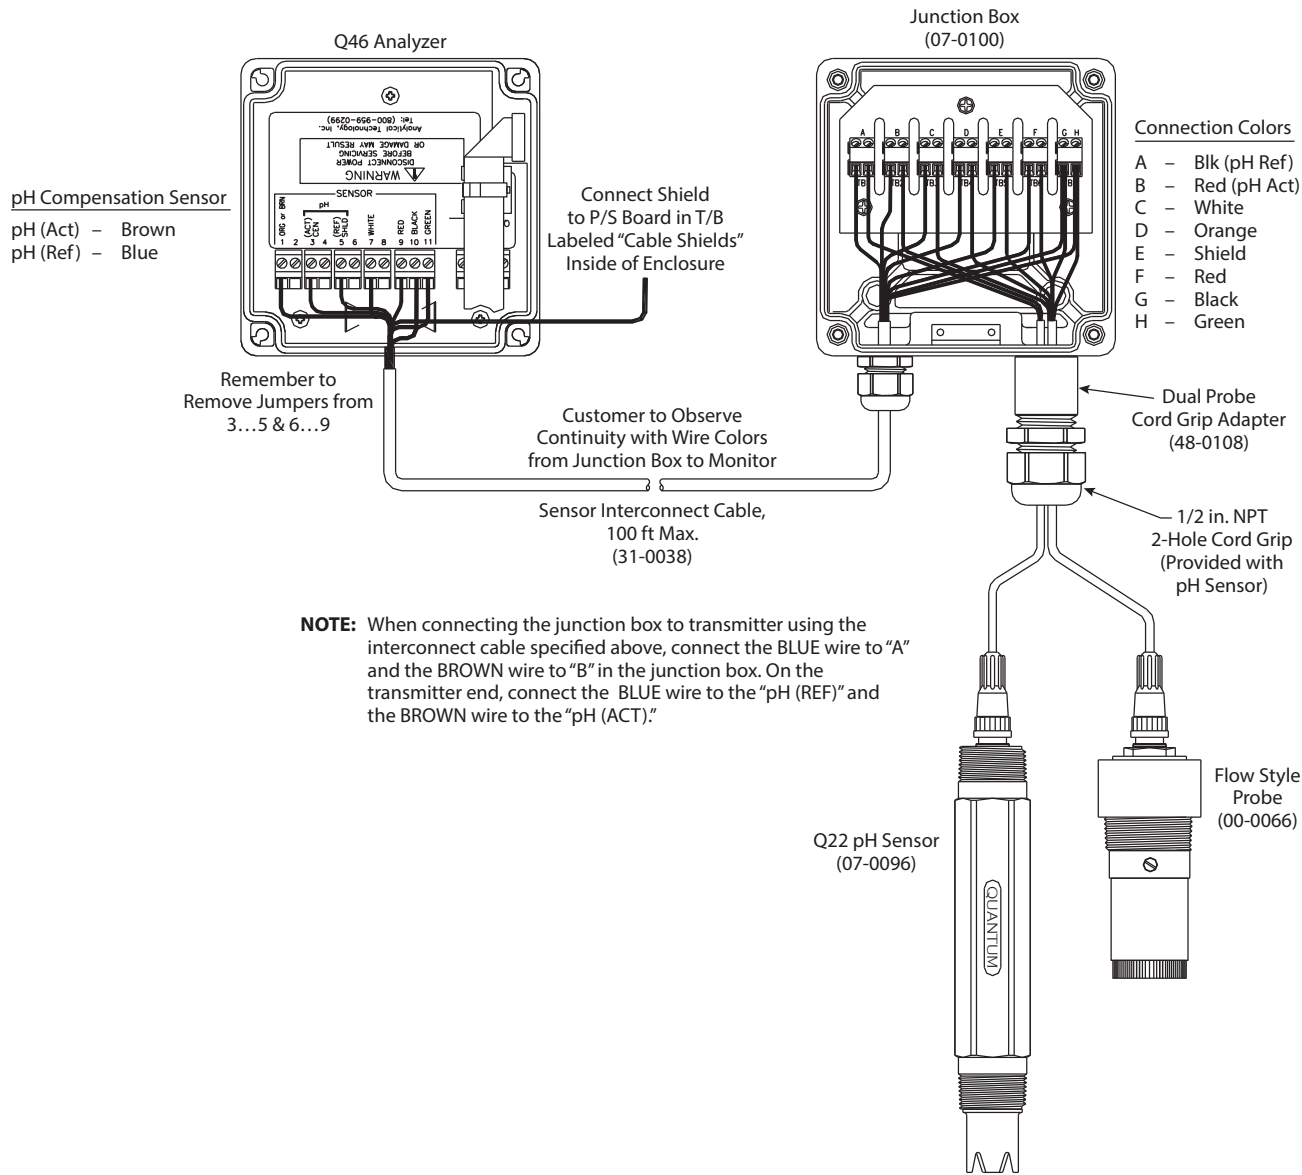

ATI-0936

**INTENTIONAL BLANK PAGE**

**INTENTIONAL BLANK PAGE**

