


ENCLOSURE DIMENSIONS

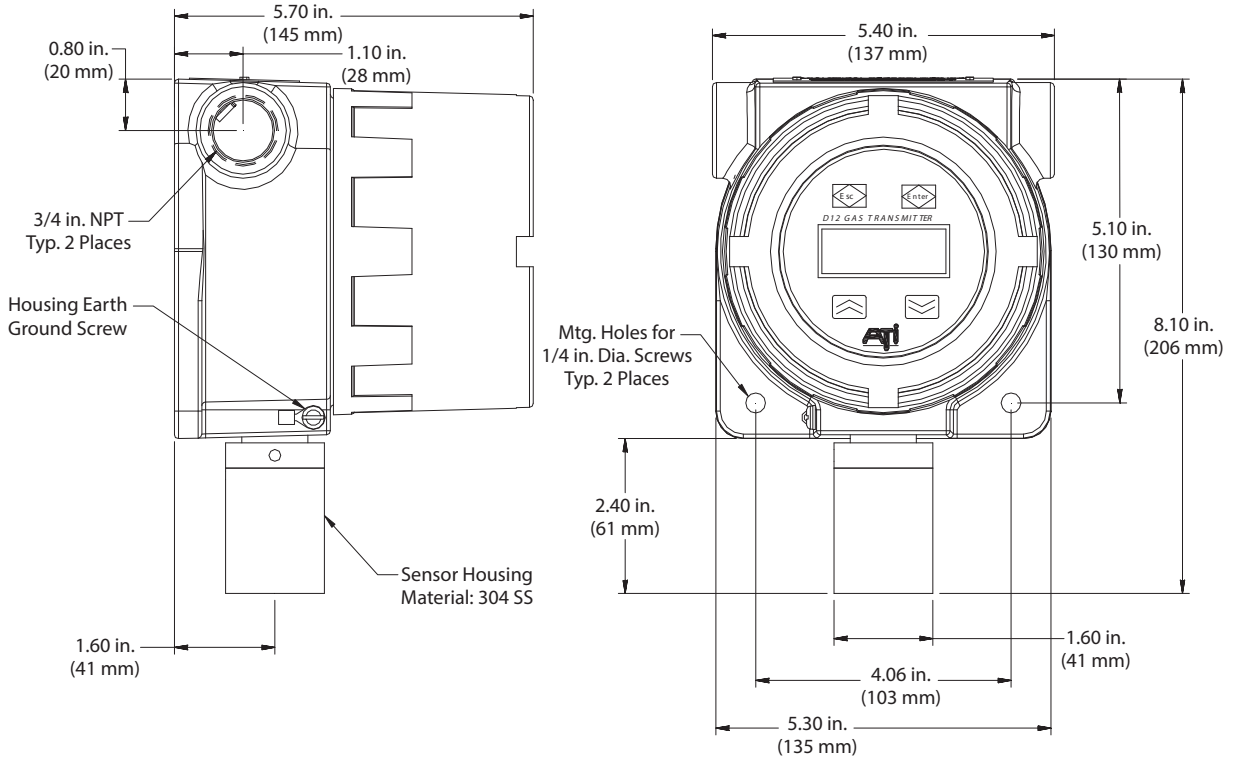


Notes:

- Enclosure Matl: Sand Case copper-free aluminum
O'Brien yellow in color.
Cover: Sand Case copper-free aluminum
O'Brien yellow in color with 3-5/16 in. dia. glass window
- Certifications:
DEMKO 18 ATEX 2066X
CE 0539 Ex II 2 G Ex db IIC T6 Gb
- EN 60079-0:2012+A11:2013
- EN 60079-1:2014


IEC Ex UL 18.0080X
Ex db IIC T6 Gb
- IEC 60079-0 (2011-06) + Corr. 1 (2012-01) + Corr. 2 (2013-12) + I-SH 02 (2014-10)
- IEC 60079-1, 7th Edition (2014-06)
- Ratings:
UL Class I, Groups B, C, D
Class II, Groups E, F, G
CENELAC: EExd IIC, IP66
Nema 4X, 78CD, 9EFG

POWER SUPPLY PCB GENERAL LAYOUT

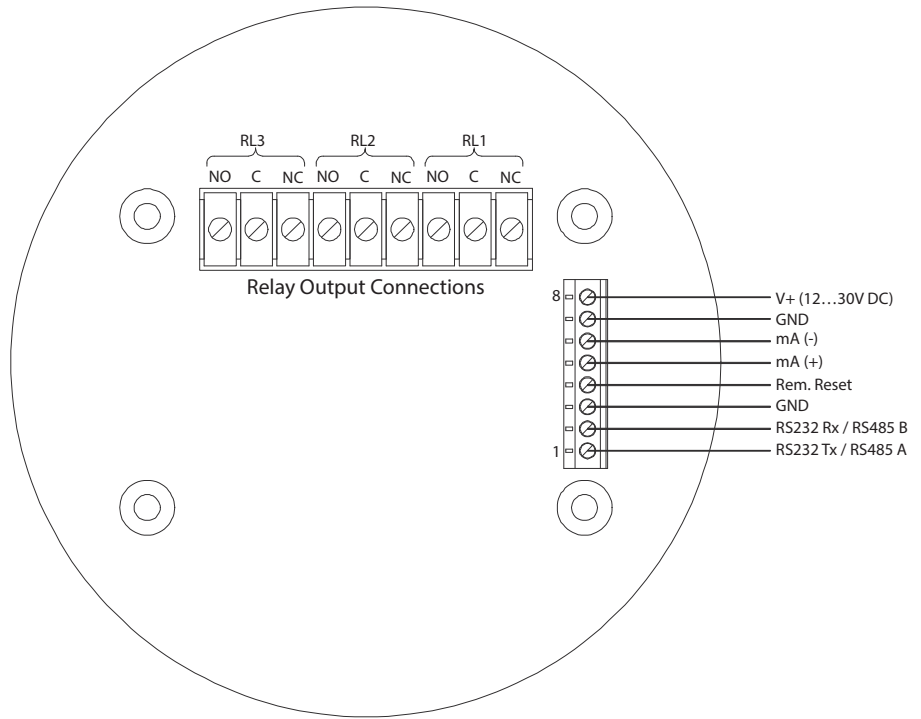


ATI-0526

3-WIRE WIRING DIAGRAM

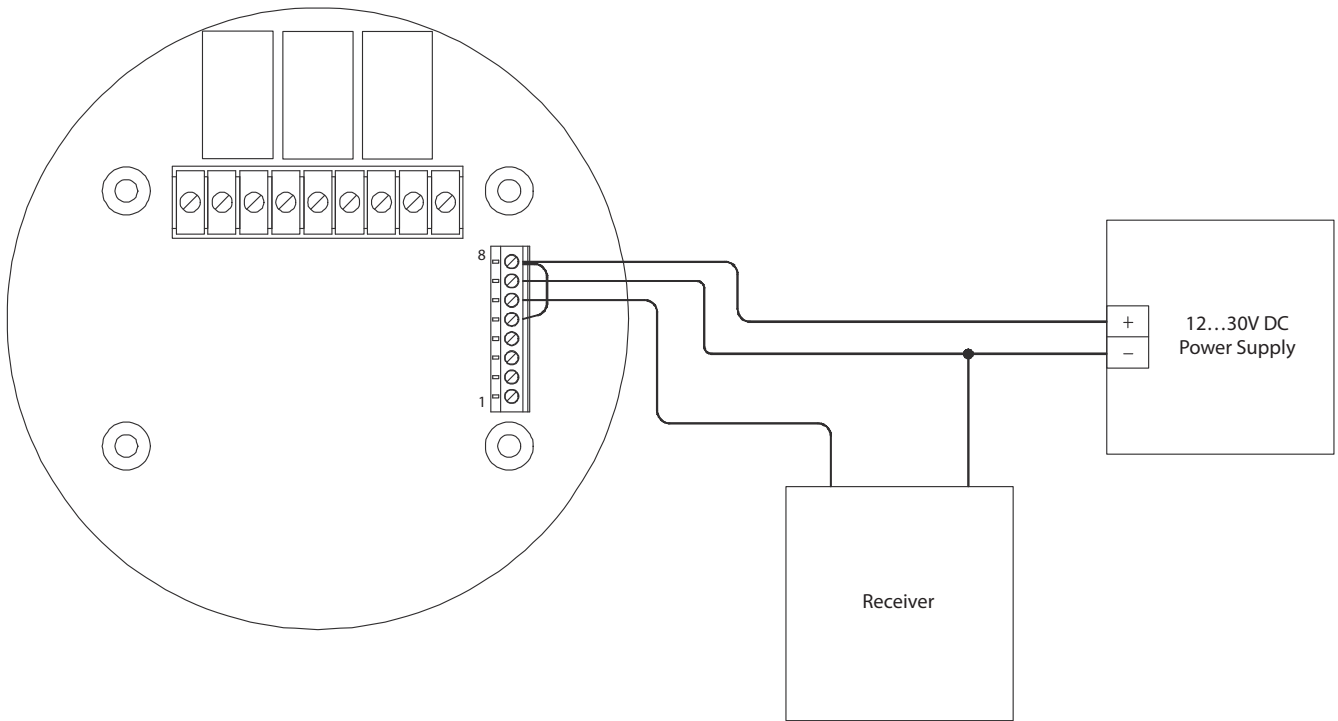

ATI-0528

REMOTE SENSOR DIMENSIONAL DRAWING

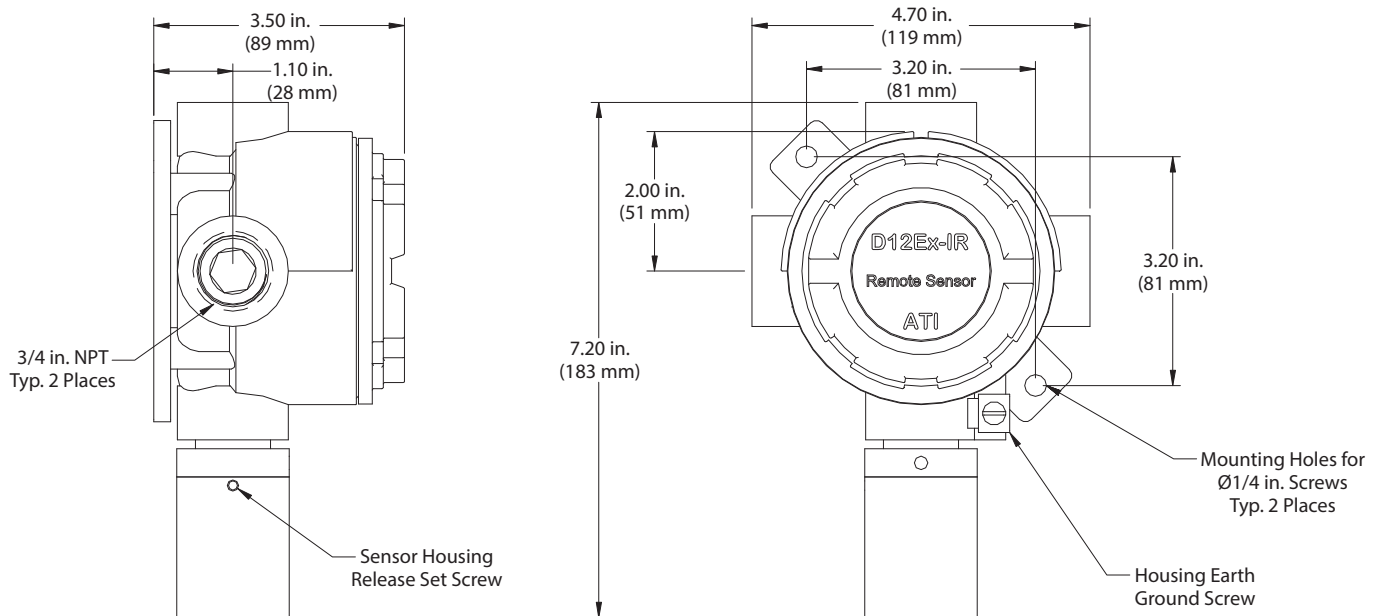


Enclosure Ratings:

Class I, Groups B, C, D
 Class II, Groups E, F, G
 Class III

Assembly is normally mounted directly to suitable explosion-proof conduit. To maintain the explosion-proof integrity of the transmitter, a suitable cable entry seal must be used in accordance with the applicable electrical code.


ATI-1204

REMOTE SENSOR WIRING DIAGRAMS

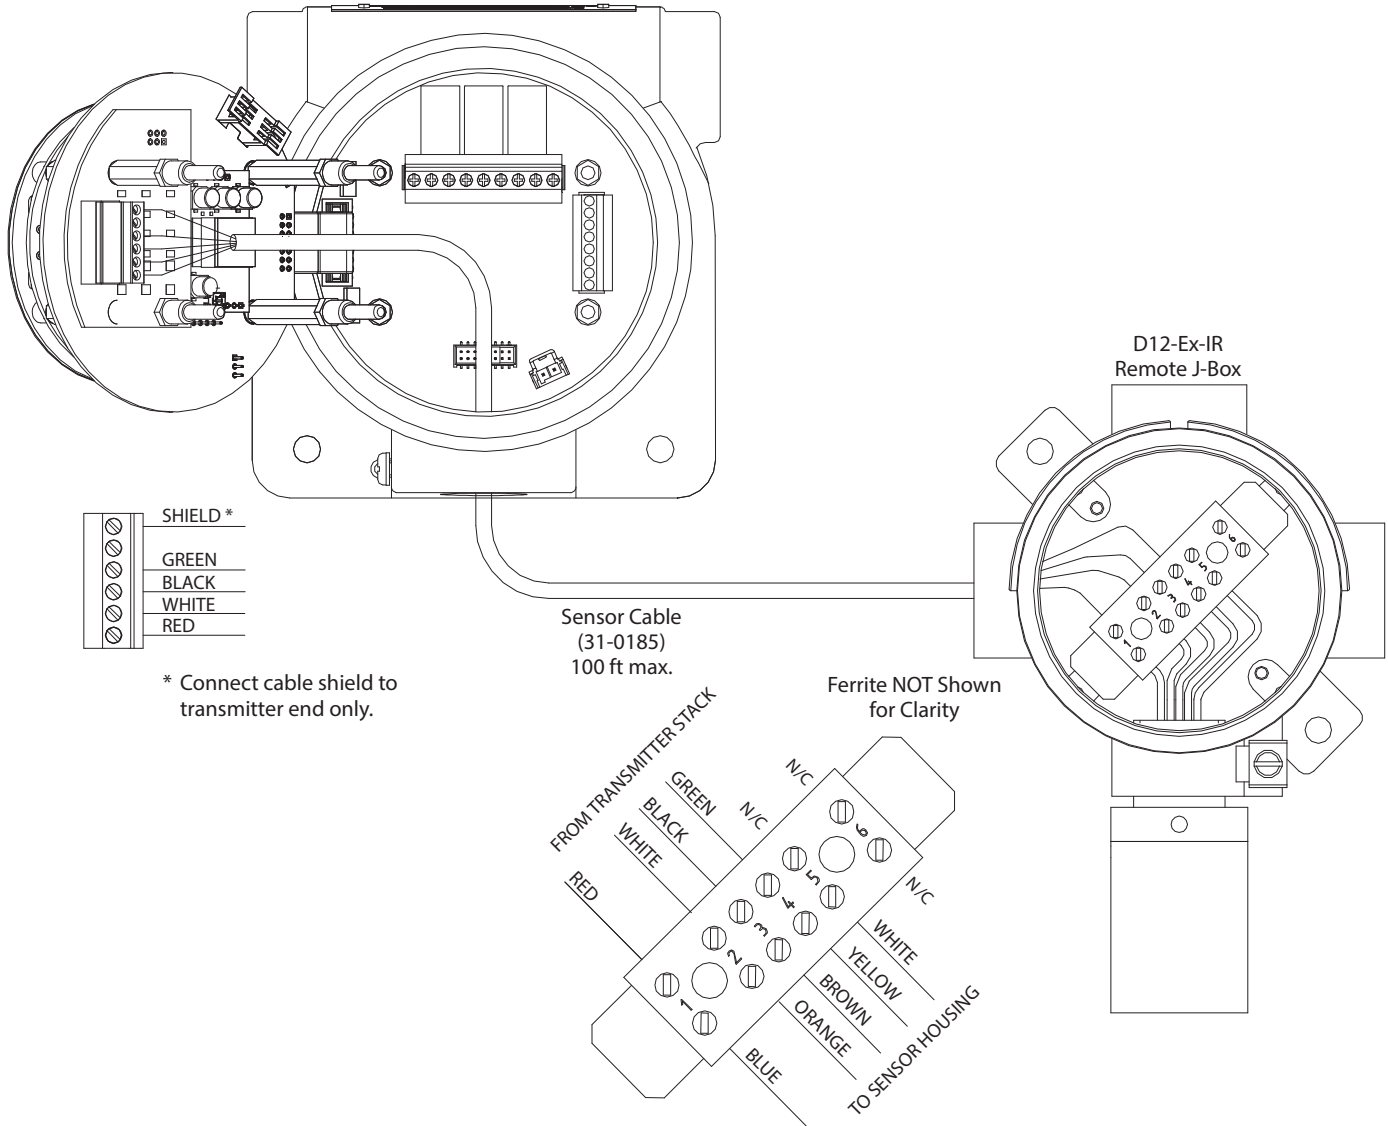


ATI-1205

FLOW CELL / CALIBRATION ADAPTER (60-0069)

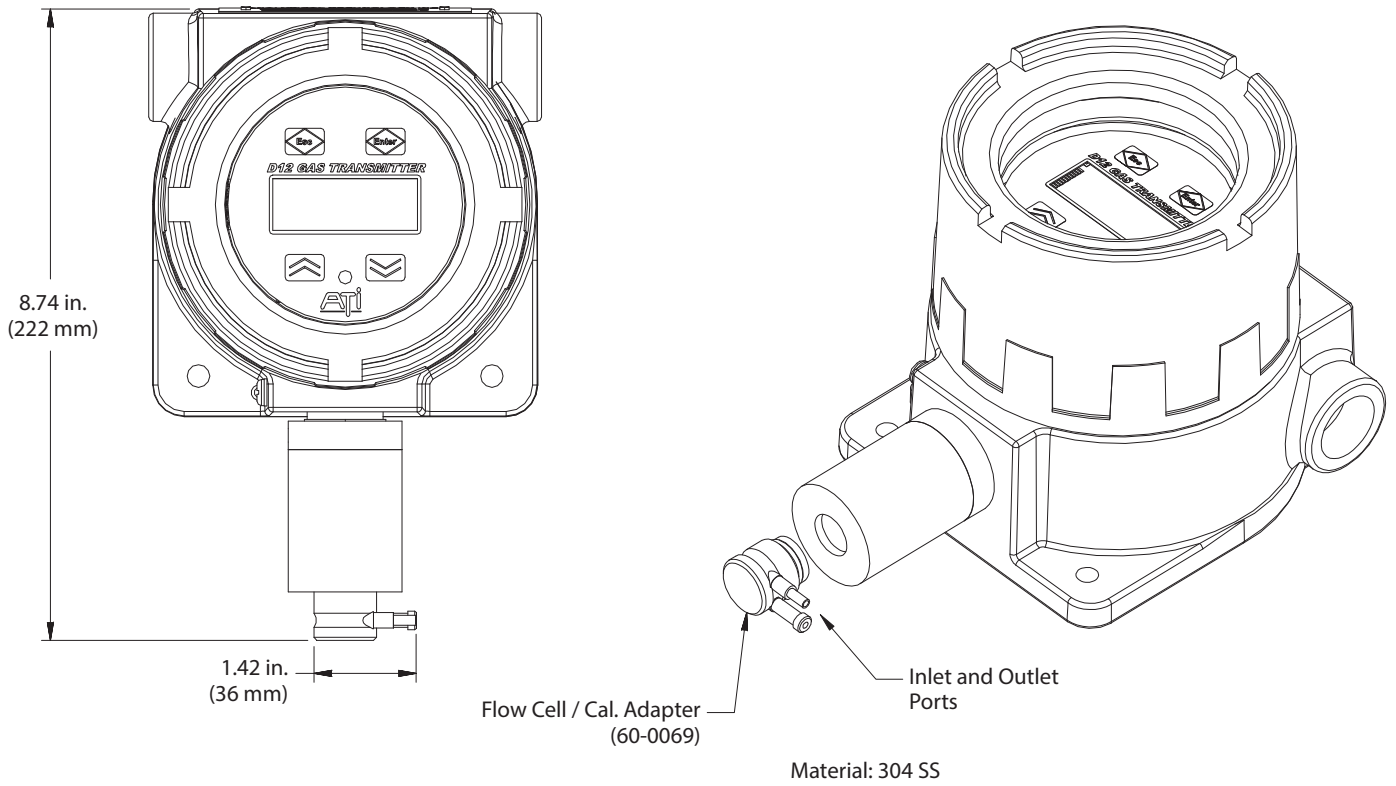

RAIN SHIELD (60-0068)

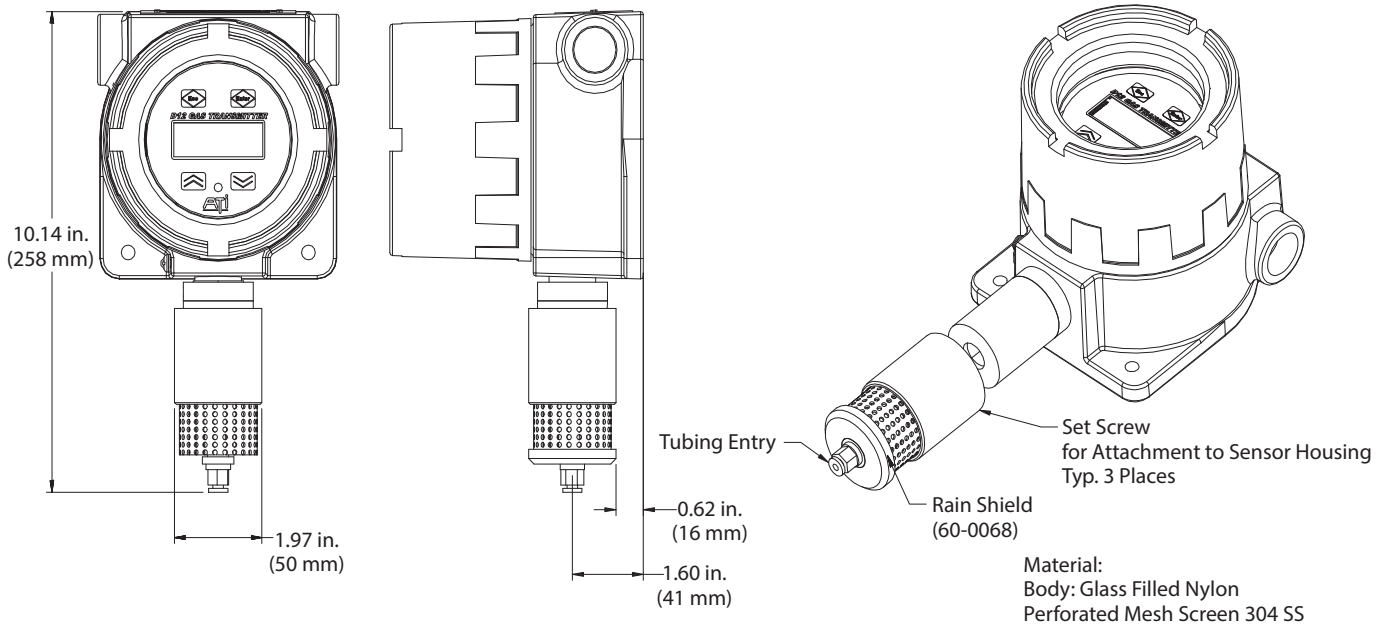

INTENTIONAL BLANK PAGE

INTENTIONAL BLANK PAGE

